


Positive
Intensity:

CJC 1295 No DAC

MS Spectrum

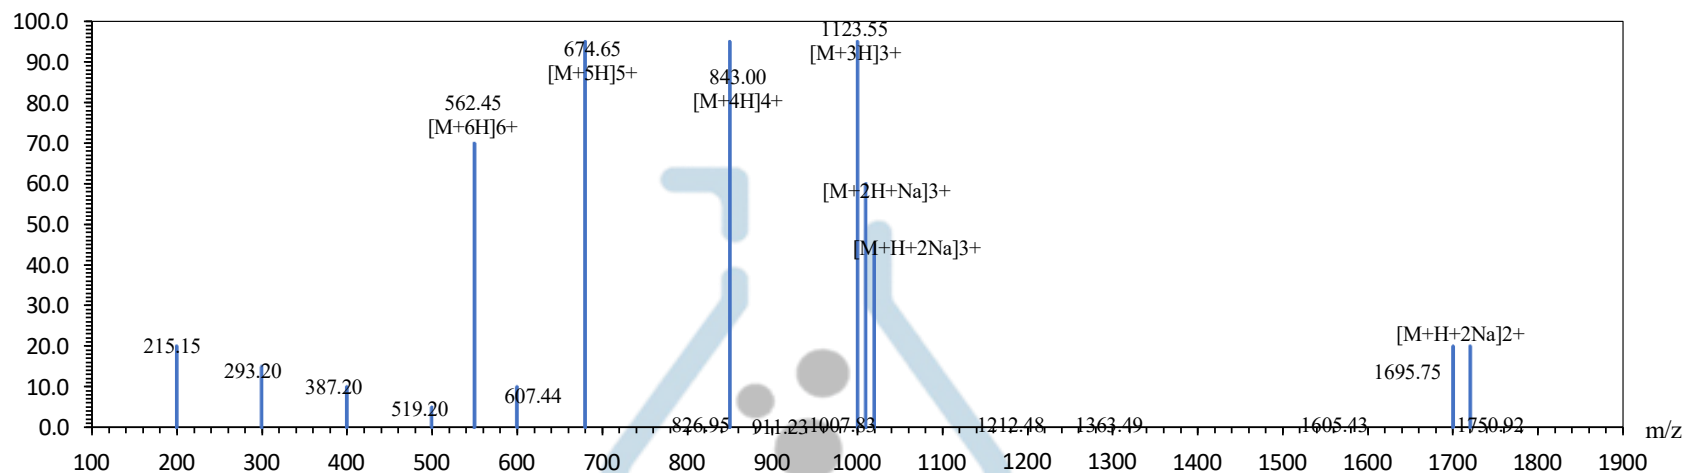

Sample Information

Dissolution method : 3% HAC+25%ACN+72%H₂O
Date Acquired : 07/06/26
Injection Volume : 1ul

Interface

Nebulizing Gas Flow : 1.50L/min
CDL Temp : 250C
CDL Volt : 0v
Block Temp : 200

Perod Bais

Detector : -0.2 kv
T.Flow : 0.2 ml/min
B.conc : 30%H₂O/70%MeOH

Lot No.

CJC01005 - CJC01028

Theoretical

3357.92

Observed

3357.65