


# HPLC

Order ID USCLBPC98661  
Lot. No BPC00210 – BPC00986  
Pump A 0.1% trifluoroacetic in 100% water  
Pump B 0.1% trifluoroacetic in 100% acetonitrile  
Total Flow 0.8ml/min  
Wavelength 220nm  
Analytical column type Phenomenex Luna 3um C18 (2) (4.6\*150mm\*3um)  
Dissolution method 100% H<sub>2</sub>O  
Acquisition Time 7/6/2026  
Inj. Volume 20ul

| Time | Module     | Action | Value |
|------|------------|--------|-------|
| 0.01 | Pumps      | B.Conc | 12    |
| 25   | Pumps      | B.Conc | 37    |
| 30   | Pumps      | B.Conc | 90    |
| 31   | Controller | Stop   |       |

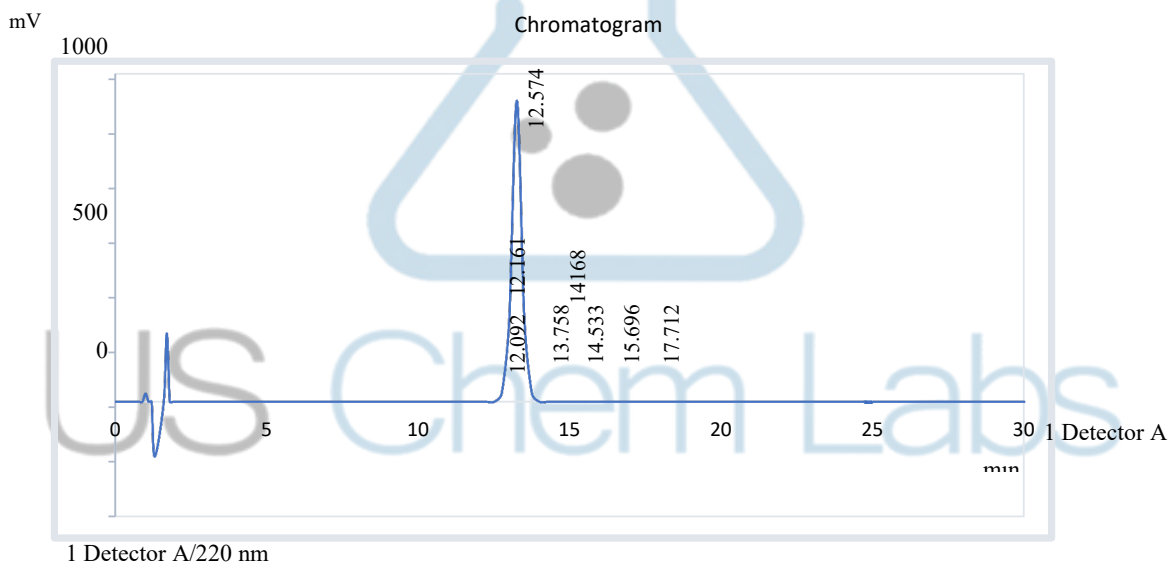

## PeakTable

Detector A 220nm

| Peak# | Ret. Time | Area     | Height | Area % |
|-------|-----------|----------|--------|--------|
| 1     | 12.092    | 82506    | 9377   | 0.202  |
| 2     | 12.161    | 94195    | 10466  | 0.203  |
| 3     | 12.574    | 16135827 | 808939 | 99.01  |
| 4     | 13.754    | 8990     | 868    | 0.055  |
| 5     | 14.168    | 69399    | 4399   | 0.212  |
| 6     | 14.533    | 8534     | 742    | 0.042  |
| 7     | 15.696    | 17833    | 1319   | 0.21   |
| 8     | 17.712    | 11707    | 954    | 0.065  |
| Total |           | 16428991 | 837064 | 100.00 |