


MS Spectrum

Scan ES+
5.62e6

Positive Intensity: **Selank**
P200305-A022 10 (10:14)

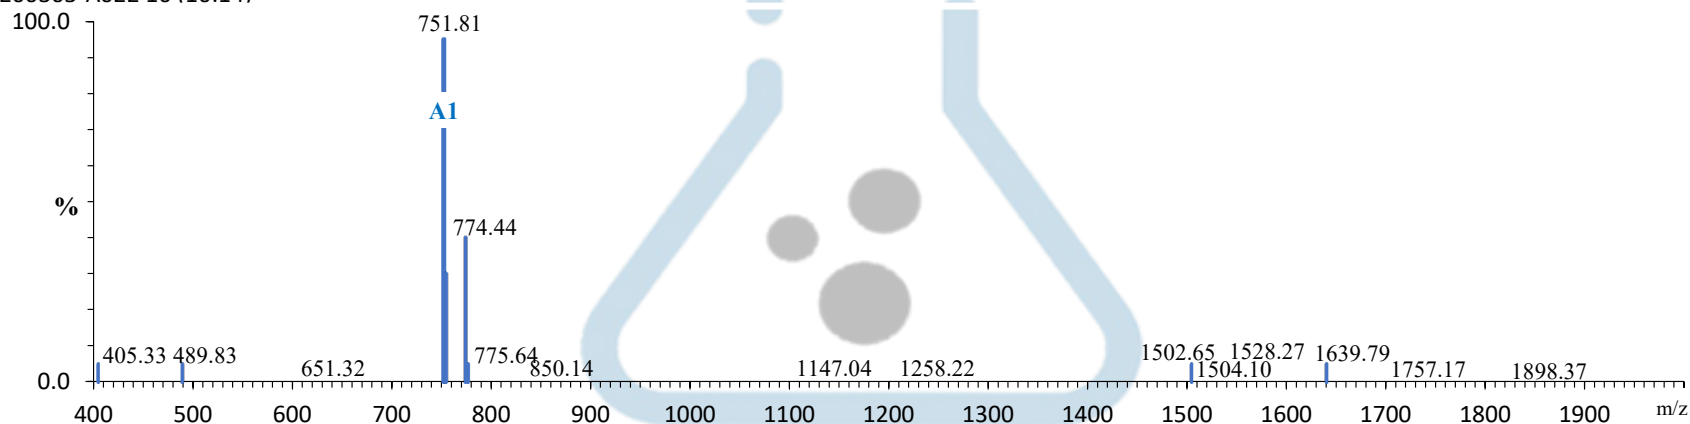

Dissolution : 0.1% HCOOH+CAN
Date Acquired : 7/6/2026
Injection : 2.5ul
Block Temp : 150
Lot. No : SEL00256 - SEL00987
Order ID : USCLSELA74531
Name : Selank
Sequence : Thr-Lys-Pro-Arg-Pro-Gly-Pro

Interface : ESI
Nebulizing Gas Flow : 500L/hr
CDL Temp : 400C
CDL Volt : 0v

Perod Bias : +3.5kv
Detector : -0.2kv
T.Flow : 0.35ml/min
B.conc : 50%H₂O/50%MeOH

Theoretical : 751.89
Observed : 751.81