


HPLC

Order ID: USCLSEMA98653
Lot. No: SEM05690 - SEM08956
Pump A: 0.1% trifluoroacetic in 100% water
Pump B: 0.1% trifluoroacetic in 100% acetonitrile
Total Flow: 0.8ml/min
Wavelength: 220nm
Analytical column type: 3u C18 (2) (4.6*150mm*3um)
Dissolution method: 100% H₂O
Acquisition Time: 7/6/2026
Inj. Volume: 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	45
25.00	Pumps	B.Conc	70
30.00	Pumps	B.Conc	90
31.00	Controller	Stop	

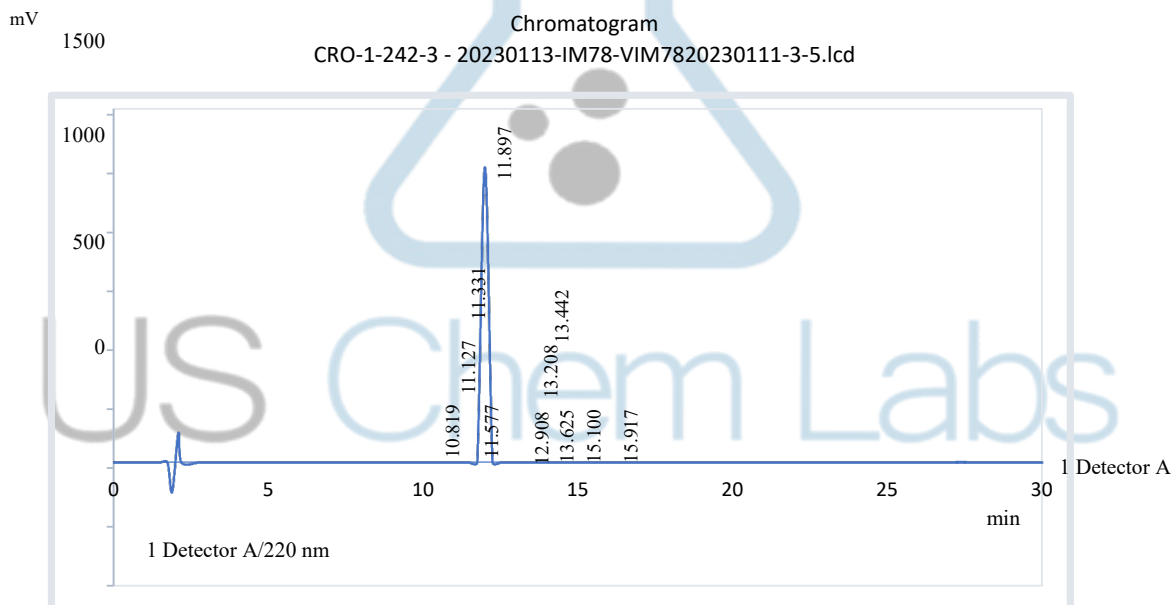

PeakTable

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.819	9642	955	0.097
2	11.127	7268	1168	0.073
3	11.331	13349	1816	0.134
4	11.577	41946	3541	0.422
5	11.897	9865824	1014126	99.151
6	12.908	1536	223	0.015
7	13.208	4668	386	0.049
8	13.442	2189	349	0.025
9	13.625	1158	133	0.012
10	15.1	1005	166	0.010
11	19.917	1242	210	0.012
Total		9949827	1023073	100.000



US Chem Labs